













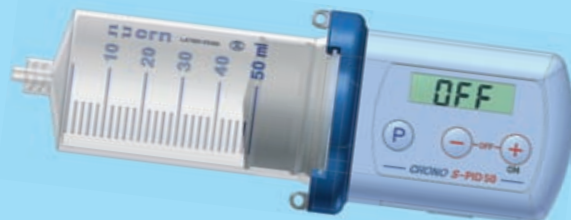

















CRONO S-PID 50

Ambulatory infusion pump

SHORT INSTRUCTIONS



Press the pushbuttons for a few seconds to activate the commands.

	ACTIVATION	BUTTONS	DISPLAY
BATTERY INSERTION	<ul style="list-style-type: none"> • Display segment complete switching on • Firmware version display • Program type display (flow rate/time) • Access to the selection flow rate/time (only possible with L 0 access level) • Flow rate/time parameter variation • Automatic positioning of the pushing unit at the infusion start • Switching off the pump 	  	      
PUMP OFF	<p>Operations only possible with L 0 access level.</p> <ul style="list-style-type: none"> • Access to the infusion end alarm selection • Access to the number of infusion sites selection (if -F- is selected) • Access to the partial volume selection <p>Variation of the value of the previous parameters</p>	 1 st depression  2 nd depression  3 rd depression 	    
PUMP OFF	<ul style="list-style-type: none"> • Viewing the infusion number performed • Anticipated withdrawal of the pushing unit • When switching on the pump, the display shows in sequence: <ul style="list-style-type: none"> - The partial volume (if programmed) - The number of infusion sites (if -F- is selected) - The programmed flow rate (if -F- is selected) - The programmed duration (if -t- is selected) - The duration of the infusion 	  and depress simultaneously 	      

	FUNCTIONS	BUTTONS	DISPLAY
PUMP ON	<ul style="list-style-type: none"> When the pump is operational the displays shows the duration of the infusion expressed in hours and/or minutes. 		5.15
	<ul style="list-style-type: none"> If a number of infusion sites is set between 2 and 5, for example 2, the pump will proceed as follows: <ul style="list-style-type: none"> - 50% of the volume of the medication contained in the syringe will be administered in the first infusion site; - at the end of the partial administration, the display will show the indication End alternating with 1-2, it is now possible to change the infusion site; - restarting the infusion, administering the remaining 50% of the medication available; - at the end of the partial administration, the display will show End and after a few seconds the pushing unit will return to the infusion start position. 	+	1P2 End 1-2 End

	FUNCTIONS	BUTTONS	DISPLAY
PUMP ON	<ul style="list-style-type: none"> Prime function 0.2 ml 	P	┆---
	<ul style="list-style-type: none"> Access to the flow rate or time value selection (with the L 0 access level) 	-	5.00 F 1
	<ul style="list-style-type: none"> Variation of the flow rate or time value 	- / +	
	<ul style="list-style-type: none"> Switching flow rate/time displays (if -F- is selected) 	+	F 1
	<ul style="list-style-type: none"> Switching off the pump 	- and + depress simultaneously	OFF

	INFUSION END	BUTTONS	DISPLAY
	<ul style="list-style-type: none"> Infusion end 		End
	<ul style="list-style-type: none"> Withdrawal positioning of the pushing unit 		┆---
	<ul style="list-style-type: none"> Switching off the pump 		OFF

Produced by:
 CANÈ S.p.A. Via Pavia, 105/i - 10090 Cascine Vica Rivoli Torino, Italy
 www.canespa.it mailbox@canespa.it



IntraPump Infusion Systems® UNITED STATES 920 Minters Chapel Road, Suite 200 Grapevine, TX 76051
 Tel: 866-211-7867 Fax: 630-845-2768 Email: info@intrapump.com